


Instructions For Use for the:

The Pink Pad[®] EXT

Prolonged Positioning System

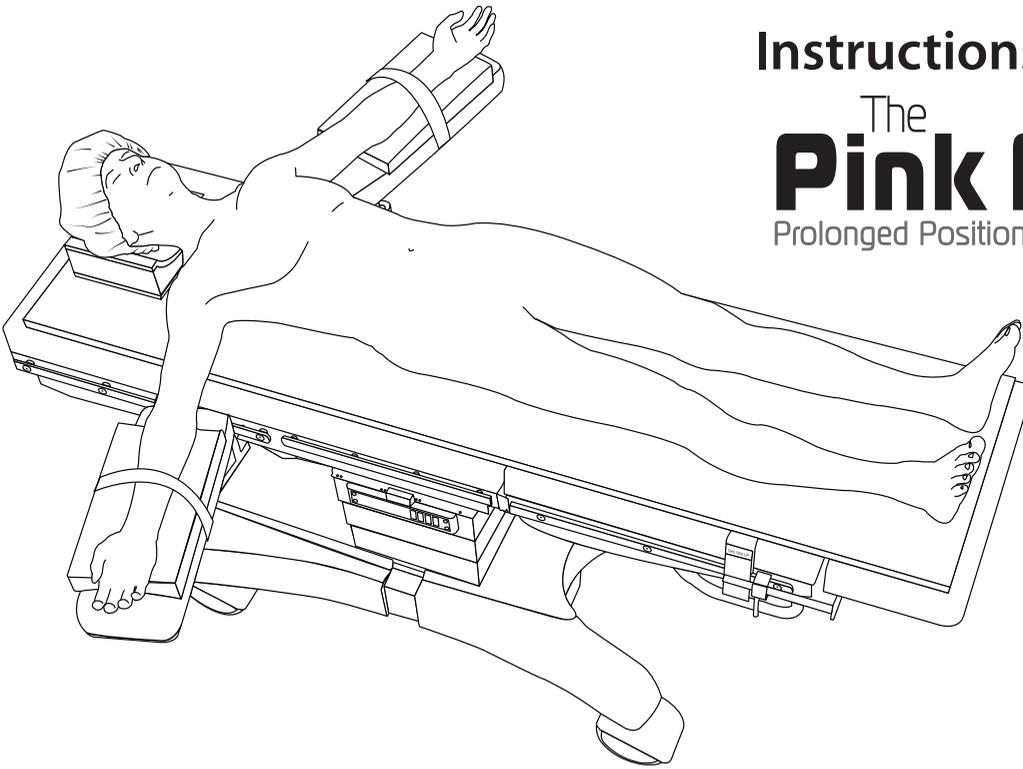

1. Place the Pink Pad EXT on the table so the white Velcro straps read "this side up". The Pink Pad EXT should be used while patient is in supine position, and warming devices can be placed under the Pink Pad EXT.
2. Attached the white Velcro straps to the surgical bed rails by looping under the rail and affixing the ends of the Velcro together.
3. Lay the lift sheet over the pad so that it is centered between the Velcro straps.
4. Follow hospital protocol for intubation. Then properly position patient on pad.
IMPORTANT: TO KEEP INTEGRITY OF THE PATIENT'S SKIN AND PREVENT PRESSURE INJURIES, THE PATIENT'S SKIN MUST MAKE DIRECT CONTACT WITH THE PINK PAD EXT. Utilize the included lift sheet to carefully lift the patient up and off the pad to repositioning as needed. Make sure pad remains completely flat at all times.
5. Lay each arm board cover with DermaProx[™] over each arm board. Position patient's arm so that the elbow and wrist rest comfortably on top of arm board cover with DermaProx[™].
6. Attach the arm board strap by wrapping it around both the arm board, arm board cover and patient's arm and looping the end of the strap through.
7. Please see reverse side for instructions on how to properly use the One-Step Arm Protectors.
IMPORTANT: NOT ALL KITS COME WITH ARM PROTECTORS.

ATTENTION:

1. Before using The Pink Pad EXT, ensure that the O.R. table pad is securely affixed to the O.R. table and is clean and free of residue
2. Be sure to follow your facility's policies and guidelines for frequency of patient monitoring. Check skin for integrity and proper circulation. Product is to be used by licensed medical professional only.
3. Care should be taken to safeguard The Pink Pad EXT from exposure to prep solutions.
4. Handling & Storage: During ALL handling and storage, assure that the pad is flat.

XODUS MEDICAL
Making Surgery Safer[™]

702 Prominence Drive
Pittsburgh, PA 15068 U.S.A.

Tel: 724.337.5500
Fax: 724.337.0555

xodusmedical.com | info@xodusmedical.com



MADE IN THE
USA

FDA REGISTERED
ISO 13485 CERTIFIED




EMERGO EUROPE
Prinsessegracht 20
2514 AP The Hague
The Netherlands

LITIFUPP011 R0 5/7/19

One-Step™ Arm Protectors

Instructions for Use

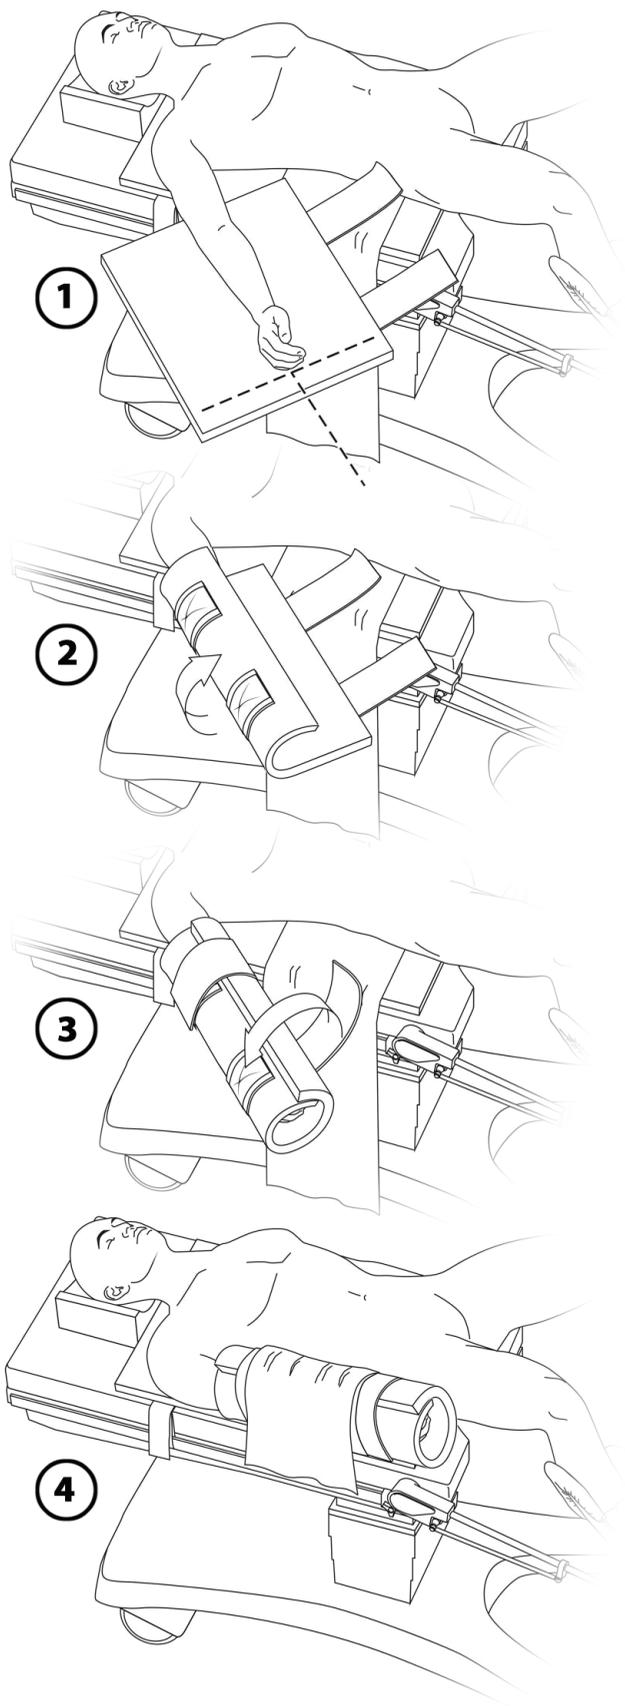

1. Place the One-Step™ Arm Protector beneath the patient's arm, centering the arm protector laterally with straps facing down and inward toward the patient's torso.

The pad should extend above the elbow and just below the fingertips. The hand should be positioned in a natural anatomical position with the palms facing inward so as not to impinge upon the ulnar nerve.

The One-Step™ Arm Protector will protect the arm, ulnar nerve and fingers while permitting easy access to the fingers and IV site. It will also safeguard against tissue breakdown.

2. Wrap the outer portion of the protector over the arm.
3. Next, wrap the remaining portion of the arm protector over the arm and secure the straps to the corresponding Velcro™ patches as shown. Ensure that the One-Step™ Arm Protector is firmly wrapped around the patient's arm.

At this stage, check for proper alignment of the wrist and fingers. Also, inspect pulse oximeters, IV lines, etc. to ensure proper placement. Accessing these patient monitors is simple and repeatable.

Repeat steps 1-3 for the remaining arm.

4. Once the One-Step™ Arm Protectors are in place, wrap the lift sheet per hospital protocol, tucking it between the patient and The Pink Pad EXT™.

Tucking methods vary according to hospital protocol. The lift sheet can be tucked either beneath the patient or beneath the O.R. table mattress. Lift sheets should not be tucked between The Pink Pad EXT™ and the O.R. table mattress.